
Reprinter RF Method

Oberon software update March 2021 comes with an additional RF option in the Reprinter section of the Analysis page.

RF = Remote Frequency



What this means is that inverted frequencies in the Reprinter page can be applied directly to the person without creating a remedy. This is an additional option to send a reprinted frequency either remotely (with a DNA sample) or while the person is present.

The process is similar to creating a remedy.


1. Begin with selecting the frequency you would like to use and click REPRINTER

* Dispersion	Inv	Thu...	Etalon
0.000			PYLORIC ANTRUM
0.923			OPTIMUM DISTRIBUTION
0.000			Virtual model
0.122			EROSIVE GASTRITIS
0.270			CATARRHAL GASTRITIS
0.794			POLYPOUS GASTRITIS
0.856			GASTROPTOSIS

2. Once on the Reprinter page select the RF option in the Matrix and change the draw count to 60 (potency of inverted frequency and number (12x5 as each draw count is 12)). Simply type in 60 into the Draw Count box

The screenshot shows the Reprinter interface. On the left, a 'MATRIX' panel contains radio buttons for WATER, ALCOHOL, SUGAR, PARAFFIN, and RF. The RF option is selected and highlighted with a red box. To the right are three buttons: EXIT, START PREPARATION, and STOP PREPARATION. Below the matrix panel, a 'DRAW COUNT' field is highlighted with a red box, containing the value '60' and a spinner control. To its right, the 'CURRENT COUNT' is displayed as '12'. At the bottom, the text 'N, N Spin=5.40, S SPIN=4.32, nQ=21.34, sQ=44.08' is visible.

3. Make sure to INVERT when appropriate (if you are not sure when to invert, take a look at the TOPICS section in the user manual). When the graph has been inverted you will see an “INV” label in the top right corner of the inverted graph.

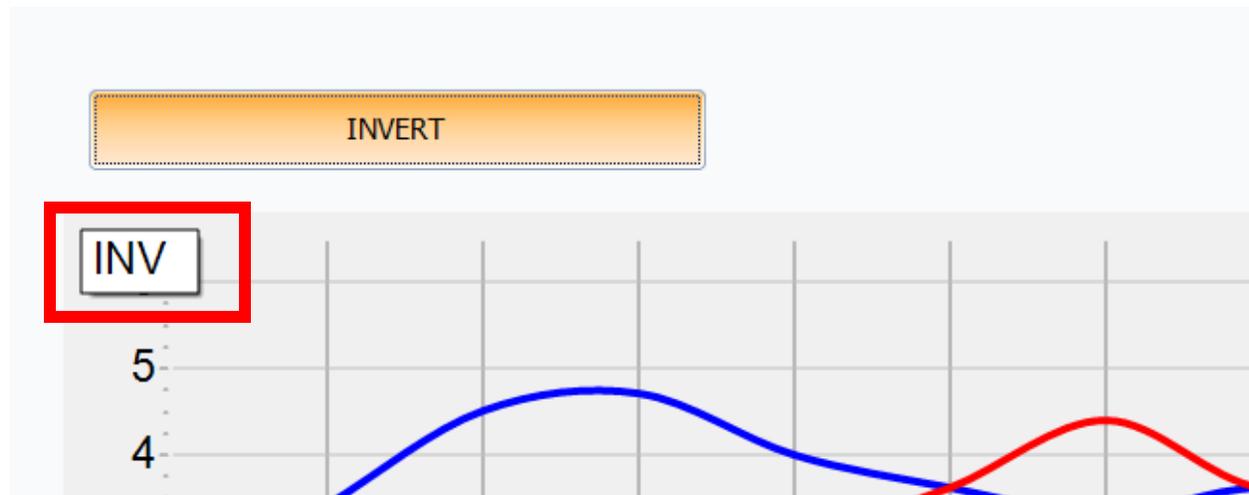


4. Before you click START PREPARATION always make sure to confirm that you have what was selected, in this case Erosive Gastritis.

The screenshot shows the 'REMEDY PREPARATION' interface. At the top, there is a color bar with a gradient from dark red to yellow. Below it, a box labeled 'EROSIVE GASTRITIS' is highlighted with a red border. To the right, a 'MATRIX' selection panel shows radio buttons for WATER, ALCOHOL, SUGAR, PARAFFIN, and RF, with RF selected. Further right are three buttons: EXIT, START PREPARATION, and STOP PREPARATION. Below the color bar, a diagram of the stomach lining is shown with various anatomical features labeled with numbers and symbols. At the bottom right, there are controls for 'DRAW COUNT' (set to 60) and 'CURRENT COUNT' (12), along with an 'INVERT' button and a scale bar.

Once you have the RF selected in Matrix, draw count changed to 60, frequency inverted when appropriate and confirmed the correct item for the Remote Frequency, click START Preparation.

This is a close-up view of the 'REMEDY PREPARATION' interface. The 'MATRIX' selection panel is visible on the left, with radio buttons for WATER, ALCOHOL, SUGAR, PARAFFIN, and RF, where RF is selected. To the right, three buttons are stacked vertically: EXIT, START PREPARATION, and STOP PREPARATION. The 'START PREPARATION' button is highlighted with a red border. At the bottom, the 'DRAW COUNT' is set to 60 and the 'CURRENT COUNT' is 12.

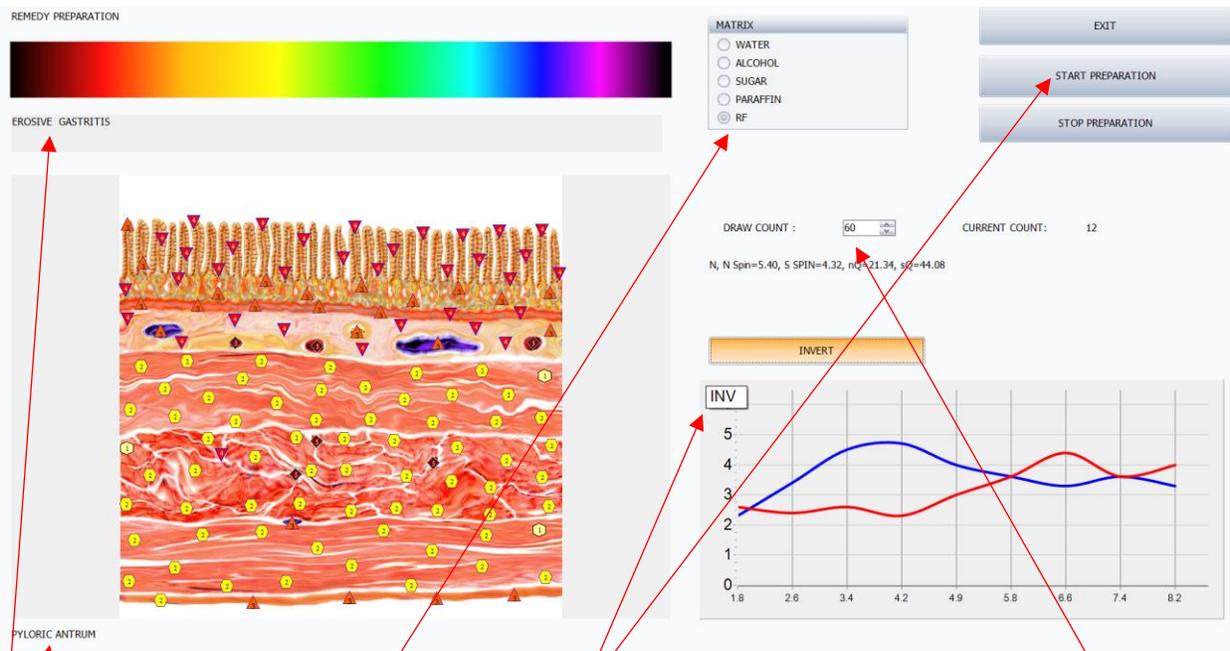

- 1 Correct item selected on the correct organ.
2. RF chosen in Matrix.
3. Draw count changed to 60 (or desired umber of rounds (each round is at a 12 draw count)).
4. Inverted when appropriate.
5. Start Preparation.

This method allows you to treat a person with an inverted frequency like a remedy does without having to take/give a remedy home. This method can be used daily or as often as you like and particularly great for pathology as microorganisms and organs have their own therapies.